

Parkview Health

Parkview Health Research Repository

Other Specialties

Parkview Research Center

10-2021

Don't Blame the Duodenoscope Elevator, the Channels Are Contaminated as Well: A Systematic Review and Meta-Analysis

Hermant Goyal MD

Sara Larsen MS

Abhilash Perisetti MD

Parkview Health, abhilash.perisetti@gmail.com

Aman Ali MD

Jiannis Anastasiou MD

See next page for additional authors

Follow this and additional works at: <https://researchrepository.parkviewhealth.org/other>



Part of the [Gastroenterology Commons](#)

Recommended Citation

Goyal, Hermant MD; Larsen, Sara MS; Perisetti, Abhilash MD; Ali, Aman MD; Anastasiou, Jiannis MD; Larsen, Nikolaj B. MS; Ockert, Lotte; Adamsen, Sven MD; Tharian, Benjamin MD; and Thosani, Nirav MD, "Don't Blame the Duodenoscope Elevator, the Channels Are Contaminated as Well: A Systematic Review and Meta-Analysis" (2021). *Other Specialties*. 36.

<https://researchrepository.parkviewhealth.org/other/36>

This Article is brought to you for free and open access by the Parkview Research Center at Parkview Health Research Repository. It has been accepted for inclusion in Other Specialties by an authorized administrator of Parkview Health Research Repository. For more information, please contact julie.hughbanks@parkview.com.

Authors

Hermant Goyal MD, Sara Larsen MS, Abhilash Perisetti MD, Aman Ali MD, Jiannis Anastasiou MD, Nikolaj B. Larsen MS, Lotte Ockert, Sven Adamsen MD, Benjamin Tharian MD, and Nirav Thosani MD

studies have documented microbes in the channels of reprocessed gastrointestinal (GI) endoscopes, including duodenoscopes and linear echoendoscopes. Our aim is to estimate the channel contamination rate of patient-ready reprocessed GI endoscopes based on the currently available data.

Methods: We searched PubMed, Web of Science, and Embase from January 1, 2010, until October 10, 2020, for studies investigating contamination rates of channels of patient-ready flexible GI endoscopes by following the PRISMA guidelines. A random-effects model based on the proportion distribution was used to calculate pooled total contamination rate. A subgroup analysis was carried out for studies originating from North America (USA and Canada). We used the meta-package (*metafor*) in RStudio version 3.6.2 to conduct the statistical analyses. Heterogeneity between the included studies was analyzed using the inconsistency index (I^2) statistics. Publication bias was assessed using funnel plots and Egger's regression tests.

Results: We identified 1,230 peer-reviewed studies after duplicates were removed. Finally, 20 studies fulfilled the inclusion criteria, including 1,059 positive cultures from 7,903 samples. The total weighted contamination rate was 19.98% \pm 0.024 (95% CI: 15.29%-24.68%; $I^2=98.6\%$) (figure 1a). Subgroup analysis amongst studies from North America (n=7) showed a contamination rate of 6.01% \pm 0.011 (95% CI: 3.88%-8.15%; $I^2=89.3\%$) (figure 1b). I^2 indicated high heterogeneity. Egger's regression test indicated no significant publication bias for both groups (Egger's test of publication bias: $p=0.0531$ and $p=0.0655$).

Conclusion: Our analysis demonstrates that 19.98% of reprocessed patient-ready GI endoscopes may be contaminated. The contamination rate was lower amongst US studies, which may be attributed to the actions taken in the US to overcome this issue. However, our findings highlight that the elevator mechanism is not the only obstacle when reprocessing endoscopes. More studies are needed to fully determine the role of contaminated endoscope channels in the cross-transmission between the patients.

S992

Don't Blame the Duodenoscope Elevator, the Channels Are Contaminated as Well: A Systematic Review and Meta-Analysis


Hemant Goyal, MD, PGDCA (MBA)¹, Sara Larsen, MSc², Abhilash Periseti, MD³, Aman Ali, MD⁴, Jiamis Anastasiou, MD, DMSc, FEBGH⁵, Nikolaj B. Larsen, MSc⁵, Lotte Ockert⁶, Sven Adamsen, MD⁷, Benjamin Tharian, MD, MRCP, FRACP³, Nirav Thosani, MD, MHA⁸.
¹Wright Center for Graduate Medical Education, Scranton, PA; ²Ambu A/S, Ballerup, Hovedstaden, Denmark; ³University of Arkansas for Medical Sciences, Little Rock, AR; ⁴The Commonwealth Medical College, Wilkes-Barre, PA; ⁵Ambu A/S, Frederiksberg, Hovedstaden, Denmark; ⁶Ambu, Ballerup, Hovedstaden, Denmark; ⁷Copenhagen University Hospital, Bispebjerg, Copenhagen, Hovedstaden, Denmark; ⁸University of Texas Health Science Center, Houston, TX.

Introduction: The elevator mechanism has been suggested as the main reason for multiple outbreaks associated with contaminated reusable patient-ready duodenoscopes. The elevator is difficult to clean even with all precautions, and specially designed brushes are recommended for proper cleaning. However, the narrow channels of the duodenoscope might pose a risk of contamination since they are prone to scratches by the insertion of various accessories creating space for microbes to hide. Our aim is to estimate the contamination rate beyond the elevator of duodenoscopes based on currently available literature.

Methods: We searched PubMed, Web of Science, and Embase from January 1, 2010, until October 10, 2020, for studies investigating contamination rates of reprocessed duodenoscope channels and areas beyond the elevator. A random-effects model (REM) based on the proportion distribution was

[0992] Table 1. Study characteristics of included studies.

First author, year	Study design	Country	Sampled channels/areas	Positive cultures, n	Sample size, N	Type of microorganism
Snyder, 2017	Parallel group randomized study	USA	Working channel	9	516	N/A
Rauwers, 2018	Prospective nationwide cross-sectional study	Netherlands	Biopsy channel, suction channel	9	283	Yeasts, Moraxella spp., Klebsiella pneumoniae, Streptococcus salivarius, Enterobacter cloacae, Moraxella osloensis, Escherichia coli, Streptococcus mitis, Klebsiella oxytoca, Neisseria flavescens, Enterococcus faecium, Rothia spp., Enterococcus faecalis, Streptococcus mutans, Pseudomonas aeruginosa, Streptococcus oralis, Staphylococcus aureus, Streptococcus spp. Bacillus spp., Stenotrophomonas maltophilia, Micrococcus luteus, Acinetobacter spp., Staphylococcus epidermidis, Agrobacterium radiobacter, Kocuria spp., Paracoccus yeeti, Staphylococcus hominis, Achromobacter xylosoxidans, Staphylococcus warneri, Alternaria spp., Kocuria rhizophila, Pseudomonas monteilii, Micrococcus spp., Pseudomonas putida, Staphylococcus auricularis, Sphingomonas paucimobilis, Staphylococcus spp. (CNS), Rhizobium spp. Or Sphingobium spp.
Olafsdottir, 2017	Parallel group randomized study	USA	Working channel	52	390	N/A
Paula, 2015	Descriptive study	Austria	Air, water, suction, and biopsy channel	47	412	Unspecified skin bacteria and aerobic spore-forming bacilli
Mark, 2020	Descriptive study	USA	Working channel	6	117	Pseudomonas aeruginosa, fungal organisms, Staphylococcus aureus, Coagulase negative staphylococcus, Viridans streptococcus
Cristina, 2020	Descriptive study	Italy	Distal end, instrument channel	35	62	Pseudomonas aeruginosa, Klebsiella pneumoniae, Acinetobacter baumannii, Klebsiella oxytoca, Stenotrophomonas maltophilia, Escherichia coli, Citrobacter freundii, Enterobacter spp
Chang, 2019	Descriptive study	Taiwan	Distal end outer surface, distal attachment cap, elevator wire channel, suction biopsy channel	43	135	N/A
Becq, 2019	Prospective single-center study	USA	Working channel	14	174	N/A

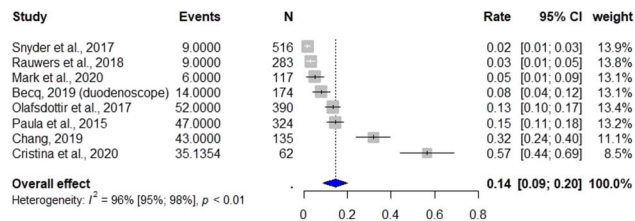

[0992] Figure 1. Pooled estimates of contamination rates beyond the elevator of patient-ready duodenoscope. CI: confidence interval; prop: proportion.

used to calculate the pooled total contamination rate beyond the elevator of reprocessed duodenoscopes. The meta-package (*metafor*) in RStudio version 3.6.2 was used to conduct the statistical analyses. Heterogeneity between the included studies was analyzed using the inconsistency index (I^2) statistics. Publication bias was assessed using the funnel plot and Egger's regression test.

Results: Eight studies including 215 positive cultures from 2,001 samples fulfilled the inclusion criteria. Four studies (50%) originated from the US, 3 studies (37.5%) originated from Europe (Italy, Netherlands, and Austria), and 1 study (12.5%) was conducted in Taiwan. See table 1 for baseline characteristics of the included studies. The total weighted contamination rate was 14.41% \pm 0.029 (95% confidence interval [CI]: 8.70% - 20.13%), see figure 1. I^2 was 96.4% indicating high heterogeneity. Egger's regression test indicated no significant publication bias (Egger's test of publication bias: $p=0.9919$).

Conclusion: Our analysis indicates that 14.41% of reprocessed patient-ready duodenoscopes may be contaminated unrelated to the elevator. These findings highlight that the elevator mechanism is not the only part of the duodenoscope, which could remain contaminated even after reprocessing. Despite the role of contaminated channels has been studied, more evidence is needed to fully determine the consequences and potential link to patient-to-patient infections. Additionally, guidelines for disinfection units should recommend through surveillance of the endoscope channels to minimize endoscope-related infections.

S993


Continued Aspirin Use and Bleeding Risk After Endoscopic Submucosal Dissection of Gastric Neoplasms: A Meta-Analysis

Hemant Goyal, MD, PGDCA (MBA)¹, Sonali Sachdeva, MBBS², Abhilash Periseti, MD³, Mark M. Aloysius, MD, PhD⁴, Saurabh Chandan, MD⁴, Benjamin Tharian, MD, MRCP, FRACP³, Nirav Thosani, MD, MHA⁵.
¹Wright Center for Graduate Medical Education, Scranton, PA; ²Boston University Medical Center, Boston, MA; ³University of Arkansas for Medical Sciences, Little Rock, AR; ⁴Creighton University School of Medicine, Omaha, NE; ⁵University of Texas Health Science Center, Houston, TX.

Introduction: With the development of endoscopic technologies, the detection rate of early gastric cancer (EGC) and precancerous lesions is gradually increasing. As an effective minimally invasive therapy, endoscopic submucosal dissection (ESD) has been accepted as a standard treatment for EGC and dysplasia. However, postprocedural bleeding is one of the most common complications of ESD, with a reported incidence of 5.1%. Moreover, the effect of continued low-dose aspirin (LDA) on bleeding during the peri-ESD period is not clear.

Methods: We searched the OVID/Medline and Google Scholar databases through June 2021 to find studies relating to continued LDA use in patients undergoing ESD. Studies reporting bleeding rates in patients undergoing ESD with and without continued LDA were included. Postoperative bleeding rates were compared between those who continued LDA during the procedure and those who did not; a random-effects model was used to calculate pooled odds ratio for bleeding risk with continued LDA use. A p-value < 0.05 was considered statistically significant.

Results: The initial search identified 2023 studies; after excluding duplicates, review articles, and studies not meeting inclusion criteria, 9 studies (all were retrospective observational studies) were finally included in the analysis. The total number of patients undergoing ESD procedure was 7978, out of which 703 continued LDA during the procedure. Pooled analysis comparing the post-operative bleeding rates between people with and without continued use of LDA revealed that aspirin use during ESD translated into higher postoperative bleeding rates compared to those who did not. (Pooled OR 1.720, 95%CI: 1.121-2.641, P= 0.01). No interstudy heterogeneity was observed ($I^2=0$).

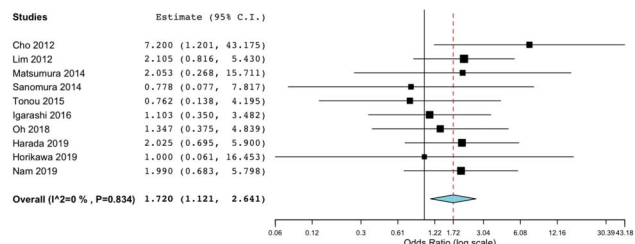

[0993] Figure 1. Forest plot of gastric neoplasm studies with and without continuation of low-dose aspirin.

Downloaded from http://ajgph.sagepub.com by BNDMSHPKAWZEDUMTICQNH4+HLZEGSHHGXMDRQWGXHMVYQJHCHD3BDCORBY77SFRG3C/V0ab9gQZkdwnt2B7rve on 10/28/2021